



Operation Instructions

Economical melt pressure sensor (transmitter)
PT111B/PT124B/PT131B/PT111/PT124/PT131series





MELT PRESSURE SENSORS CE
Ziaslot

MELT PRESSURE SENSORS CE
Ziaslot
PT124-4M-1/2-4/18

MELT PRESSURE SENSORS CE
Ziaslot
PT124-5M-1/2-6/18

MELT PRESSURE SENSORS CE
Ziaslot

MELT PRESSURE SENSORS CE
Ziaslot

齐亚斯 Ziaslot
A Heqing Group Company
400-881-0121
www.ziaslot.com

US 110 1/2 18

CONTENTS

01	Product Introduction	01
02	Product Model and Specifications	01
03	Transportation and Storage	02
04	Product Installation Hole	02
05	Product Installation	03
06	Product Disassembly	04
07	Housing Fixation	04
08	Wiring and Cabling	04
09	Product Calibration	05
10	Electrical Connection	06
11	Fault Analysis	08

01 Product introduction

The economical melt pressure sensor (transmitter) is an instrument for measuring melt pressure in high temperature areas (referred to as sensor and transmitter), with digital-analog integrated circuit design. Please store and operate according to the following instructions to ensure the maximum service life of the product. The product complies with the national JJG860-2015 "Pressure Sensor (Static) Verification Regulations" and JJG882-2019 "Pressure Transmitter Verification Regulations".

02 Product Model and Specifications

Product model: PT111 (rigid type), PT124 (Rigid+flexible type), PT131 (With thermocouple type)

2.1 High temperature melt pressure sensor (PT111/PT124/PT131)

Definition: Output signal is 2m V/V

Measuring range: (0-10) MPa, (0-20) MPa, (0-35) MPa, (0-50) MPa, (0-70) MPa, (0-100) MPa

2.2 High temperature melt pressure transmitter (PT111B/PT124B/PT1131B)

Definition: Output signal is (4-20) mA, 0-10 Vdc, 0-5 Vdc

Measuring range: (0-10) MPa, (0-25) MPa, (0-35) MPa, (0-50) MPa, (0-70) MPa, (0-100) MPa

Performance Parameter	High Temperature Melt Pressure Sensors	High Temperature Melt Pressure Transmitter	
Output Signal	3.33mV/V	(4-20)m A Two-wire system	3-wire(0-10)Vdc, 3-wire (0-5)Vdc
Supply Voltage	(6-12)Vdc (10 Vdc recommended)	(10-36)Vdc	(18-36)Vdc
Load resistance (Ω)		<(Supply voltage-10)/0.02	>10k
Calibration signal: 80% F.S.			
Basic Error (%)	$\pm 0.5\%$ (level 0.5), $\pm 0.25\%$ (level 0.25)(expressed as a percentage of the full scale output value) Repeatability shall not be greater than the absolute value of the basic error, and the return difference shall not be greater than the absolute value of the basic error.		

03 Transportation and Storage

3.1 The product is normally packaged individually and when stored, please carefully repackage the packaging it originally came with.


3.2 At the front thread of the rigid rod, the induction diaphragm is protected by a protective cap, which should be tightened at any time during storage and only opened when using the installation. It is strictly prohibited to press the diaphragm with sharp materials.

3.3 Long-term storage needs to meet the following conditions:


- ① Ambient temperature: $-20\sim 85^{\circ}\text{C}$, relative humidity: $0\%\sim 100\%\text{R.H}$
- ② Not exposed to rain or affected by water seepage/leakage.
- ③ Vibration and shock kept to a minimum.

04 Product Installation Hole

Before installing the product, make sure that the mounting holes are machined to the correct size and that the holes are free of burrs.




d1	d2	d3	d4	a	b	c
1/2-20UNF	$\Phi 8$	$\Phi 11.5$	$\Phi 14$	5.7	3.2	19
M18×1.5	$\Phi 10$	$\Phi 16.5$	$\Phi 20$	6	4	25
M10×1	$\Phi 6.2$	$\Phi 9.1$	$\Phi 14$	6.7	3.2	19
M14×1.5	$\Phi 8$	$\Phi 12.5$	$\Phi 15$	5.7	3.2	19
G1/4	$\Phi 8$	$\Phi 11.7$	$\Phi 14$	5.7	3.2	19
M12×1.5	$\Phi 8$	$\Phi 10.5$	$\Phi 14$	5.7	3.2	19



d1	d2	d3	d4	a	b	c
G3/8	$\Phi 10$	$\Phi 15$	$\Phi 18$	9	4	25
G3/4	$\Phi 18.1$	$\Phi 24.5$	$\Phi 28$	12	5	35
M22×1.5	$\Phi 16$	$\Phi 20.5$	$\Phi 24$	10	5	40
M20×1.5	$\Phi 14$	$\Phi 18.5$	$\Phi 22$	5.7	3	35

Correct Installation Mode

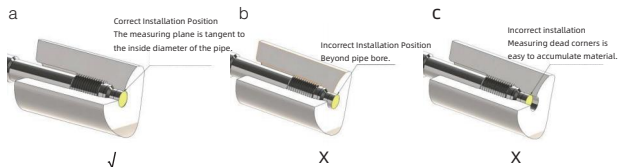

05 Product Installation

5.1 Before installing the product, please check whether the technical parameters on the nameplate are correct or not, mainly including mounting threads, pressure range, output signal, power supply requirements. The main parameters include mounting thread, pressure range, output signal and power supply requirements.

5.2 Ensure that the mounting holes are drilled to the correct dimensions. If the product is installed in a previously used mounting hole, professional cleaning tools should be used to ensure that the mounting hole is completely clean and free of any plastic residue.

5.3 Remove the protective cap from the front of the product.

5.4 Apply high-temperature anti-seize grease to the threaded surfaces of the product to prevent thread seizure. If you need to install a gasket when sealing the flat surface, please put the high temperature anti-seize grease on the surface. If you need to install a sealing gasket for flat sealing, please apply high-temperature anti-seize grease on the sealing gasket and stick the gasket on the product.

5.5 Place the product smoothly into the mounting hole, first manually, and then use a wrench to tighten it on the hexagon. If the product is to be mounted in a previously used mounting hole, it is recommended that the product be mounted under conditions of heating to the melting point of the plastic.

The recommended maximum mounting torque is 40 Nm.


06 Product disassembly

6.1 Disassembly must be done under heated conditions (plastic melting point). When disassembling the sensor, make sure that the diaphragm is not contact pressure. The force for dismantling the sensor must be applied only to the shaft (hexagon) and not to the sensor head. Do not apply any force to the sensor head. If the mounting holes need to be blocked, seal them with a plug of the same mechanical size.

6.2 After disassembling the product, the diaphragm, sealing surfaces and threads must be quickly wiped clean with a soft cloth.

07 Product disassembly

Use our professional mounting bracket to fix the product, the fixing position should avoid vibration and installation in a strong magnetic environment, and should not be exposed to rain or water seepage/leakage, the temperature should not exceed 85°C.



Please strictly follow the operation instructions to install and disassemble the product, caused by misoperation damage, we does not assume the quality responsibility.

08 Wiring and Cabling

8.1, the cable should be used with a shielded cable, heat-resistant temperature of not less than 105 °C, each core line connecting terminal should be heat-shrinkable The shielded cable should be connected with the plug-in metal, and special care should be taken when welding the cable, otherwise it may lead

to signal transmission error or damage the product. Otherwise, it may cause signal transmission error or damage the product. Please refer to "Electrical Connection" for wiring definition.

8.2. If you use our welded cables, you only need to connect them according to the definition of "Electrical Connection".

8.3 Signal cable should be wired separately through the wiring channel, strong and weak power should be wired separately, please avoid high temperature when wiring. The recommended ambient temperature is below 85°C.

8.4. It is strictly prohibited to plug the cable into the electrical connection of the high-temperature melt pressure sensing/high-temperature melt pressure transmitter, The cable should not be pulled out of the wiring.

8.5 After the cable is connected, connect it to the terminal block of the signal receiving end according to our electrical connection definition. If there is any extra If there is any extra wire core, please wrap each wire core individually with insulating tape.

09 Product Calibration

After the product is installed and connected to the measuring instrument and powered on, and in the absence of any pressure, the system temperature has reached the operating temperature 30min to 60min, the product is calibrated.

Calibration method:

- High temperature melt pressure sensor (mV/V signal output):
Please zero and calibrate the instrument on the display meter. Please refer to the zeroing method and calibration method of the display instrument.
- High temperature melt pressure transmitter:
Remove the screw with "Z" on the top of the housing, there is a button in the hole, use insulating material to press the button to realize the automatic zero function. The function of automatic zeroing can be realized by pressing the button with insulating material.

10 Electrical Connection


Pressure output signal wiring definition:

PT111/PT124/PT131

Electrical Wiring Configuration

4-Wire Transmitter

2mV/V




Connector type:XS12J5Y-5PIN.

PIN	Function	Wire Color
1	Signal+	Blue
2	Power+	Red
3	Signal-	White
4	Power-80%	Yellow
5	80%+	Black

Electrical Wiring Configuration

2-Wire Transmitter

4...20mA




Connector type:XS12J5Y-5PIN.

PIN	Function	Wire Color
1	Power-	Blue
2	Power+	Red
3	Signal-	White
4	80%	Yellow
5	80%+	Black

Electrical Wiring Configuration

4-Wire Transmitter

0...5V/10V




Connector type:XS12J5Y-5PIN.

PIN	Function	Wire Color
1	Signal +	Blue
2	Power +	Red
3	Signal -	White
4	Power-80%	Yellow
5	80%+	Black


*Pin 3 and 4 Connected internally

Cable should be used with shielded cable, each core line about 0.3mm², heat-resistant temperature of not less than 105 °C, each core line connecting terminal should be heat-shrinkable tube isolation protection, shielded wire to be connected with the plug-in metal, cable welding should be particularly careful, otherwise it may lead to signal transmission errors or damage to the product, it is recommended to use ziasiot has been welded to a good special cable line. Extra wires in the cable should be individually wrapped with insulating tape.

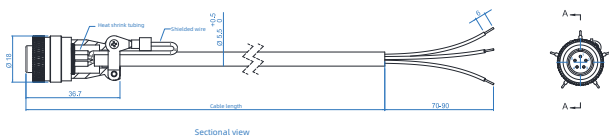


Please contact the factory for other connectors specification drawings.

Temperature signal output:





Thermocouple type		Thermocouple temperature signal	Cable color
K type thermocouple		+	Red
		-	Blue
E type thermocouple		+	Red
		-	Brown
J type thermocouple		+	Red
		-	Yellow

Temperature signal output:

		Three-wire PT100	Cable color
		+	Red
		G	Red
		-	White

11 Fault Analysis

Common faults and troubleshooting methods:

Fault	Reason	Troubleshooting Methods
	1. The hole size problem: the size is small, the concentricity is not enough, and the hole has rough edges. 2. The temperature is more than 400°C.	1. Check the hole size. 2. Check whether the normal operating temperature exceeds 400 °C or whether the temperature exceeds 400 °C during the heating process.
	1. The installation hole caused by burrs. 2. Cold machine installation, solidification caused by materials. 3. External use of hard objects to press the diaphragm.	1. Clear the burrs in the hole. 2. Use special cleaning tools to clear the hard material in the hole and install with the heating machine. 3. Only use fingers to press.
	1. The hole size problem: the diaphragm has extended out of the inner wall of the cylinder. 2. Brush the diaphragm with a hard object.	1. Re-open the hole or add the gasket according to the size. 2. It is strictly prohibited to use hard objects to brush the diaphragm.
	Excessive mounting torque.	Install according to the recommended torque, and try to make the installation force 90° with the screw.
	Reason	
Pressure did not change	1. Check whether the power supply and cable connections are correct.	
	2. Check whether the diaphragm is intact.	
	3. Check whether the output signal is consistent with the input signal of the receiving module.	
	4. Check whether the sensor housing is at a temperature below 80 °C.	
Pressure fluctuation	1. Need to use a shielded cable.	
	2. The equipment should be reliably grounded.	
	3. The shielded wire is connected to the electric control PE wire.	
Pressure measurement is not accurate	1. Check whether the power supply and cable connections are correct.	
	2. Check whether the diaphragm is intact.	
	3. Check whether the output signal is consistent with the input signal of the receiving module.	



Shanghai Ziasiot Technology Co., Ltd.

6th floor,18th Building,No.615, Lianying Road, Songjiang District, Shanghai,China.

Tel: 021-37635502 400-821-0137

Fax: 021-37635507

Email: info@ziasiot.com

Web: <http://www.ziasiot.com>(English) <http://www.ziasiot.net>(chinese)

Zias(Zhejiang) IoT Technology Co.,Ltd.

3F305, R&D Building, No.1237Jiichuang Road,Xiuzhou District,
Jiaxing City,Zhejiang province,China

Email: zias@ziasiot.com

Tel: 0573-83312892

